


User's Guide



Heavy Duty Differential Pressure Manometer

Model 407910

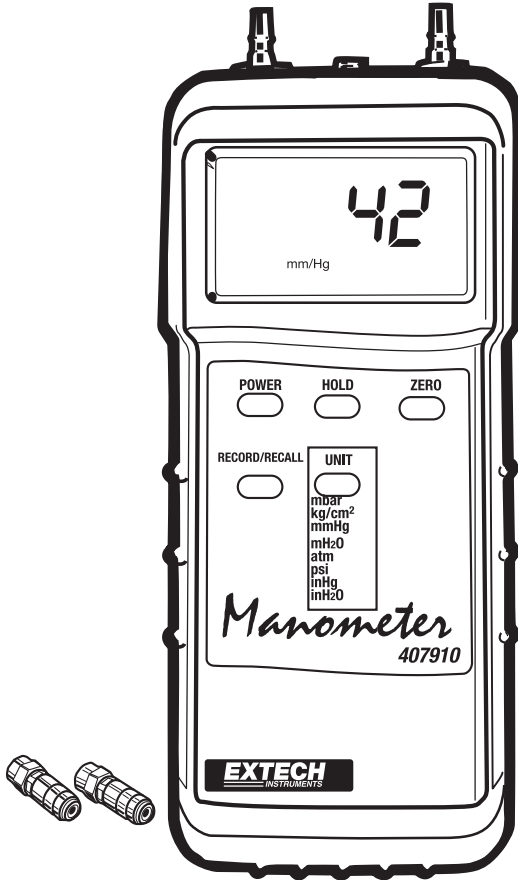

Warranty

EXTECH INSTRUMENTS CORPORATION warrants this instrument to be free of defects in parts and workmanship for **one year** from date of shipment (a six month limited warranty applies to sensors and cables). If it should become necessary to return the instrument for service during or beyond the warranty period, contact the Customer Service Department at (781) 890-7440 ext. 210 for authorization or visit our website www.extech.com for contact information. A Return Authorization (RA) number must be issued before any product is returned to Extech. The sender is responsible for shipping charges, freight, insurance and proper packaging to prevent damage in transit. This warranty does not apply to defects resulting from action of the user such as misuse, improper wiring, operation outside of specification, improper maintenance or repair, or unauthorized modification. Extech specifically disclaims any implied warranties or merchantability or fitness for a specific purpose and will not be liable for any direct, indirect, incidental or consequential damages. Extech's total liability is limited to repair or replacement of the product. The warranty set forth above is inclusive and no other warranty, whether written or oral, is expressed or implied.

Introduction

Congratulations on your purchase of the Extech Manometer Model 407910. This device has a differential input with convenient quick-disconnect fittings. Eight units of measure are selectable by front panel pushbutton. Advanced features include Data hold, MAX/MIN record/recall, and RS-232 PC interface. Properly used, this device will provide years of reliable service.

Specifications

General Specifications


Circuit	Custom one-chip LSI microprocessor circuit
Display	0.6" (16mm) 2000 count LCD with function indicators
Units of Measure	mBAR, psi, kg/cm ² , mm Hg, inches Hg, meter H ₂ O, inches H ₂ O and Atmospheres
Input circuit	Differential inputs (P1 and P2)
Data Hold	Freezes displayed reading
Sensor	Built-in piezoelectric sensors
Zero Adjust	Front panel push-button
Sample rate	0.8 sec. (approx.)
Compatibility	Air or non-corrosive and non-ionized gas
Auto Power OFF	Meter turns off after approx. 10 minutes to conserve energy
Data Output	RS-232 PC serial interface
Ambient conditions	32 to 122°F (0 to 50°C); < 80% RH
Battery power	9V alkaline battery
Power Consumption	6mA DC (approx.)
Dimensions	7.1 x 2.8 x 1.3" (180 x 72 x 32 mm)
Weight	0.76 lbs (345 g)
Accessories	Quick-disconnect fittings (2), rubber jacket, and 9V battery

Range Specifications

Range/Units (Max.)	Resolution	Accuracy
± 2000 mbar	1	± 2% full scale @ 23±5°C Note: Accuracy includes linearity, hysteresis and repeatability effects
± 29 psi	0.02	
± 2.040 Kg/cm ²	0.001	
± 1500 mm Hg	1	
± 59.05 inches Hg	0.05	
± 20.40 meters H ₂ O	0.01	
± 802 inches H ₂ O	0.5	
± 1.974 atmospheres	0.001	

Meter Description

1. LCD Display – Indicates the measurement data, unit of measure, and user alert symbols as described in this manual
2. Push-buttons:
 - POWER – Press to turn the meter ON or OFF
 - HOLD – Press to freeze the displayed reading
 - ZERO – Press to null the display (with fittings disconnected)
 - RECORD/RECALL – Press to access the MIN/MAX recording mode as described later in this manual
 - UNIT – Press to select the unit of measure
3. 0.16" (4mm) Quick-disconnect fittings (supplied)
4. P1 Input – 0.16" (4mm) accepts quick disconnect connector
5. RS-232 PC interface jack (3.5mm) – For use with data acquisition software/hardware interface kit model 407001
6. P2 input – 0.16" (4mm) accepts quick disconnect connector
7. Rubber protective holster (removable)
8. Battery compartment (on rear) – Remove rubber jacket to access compartment

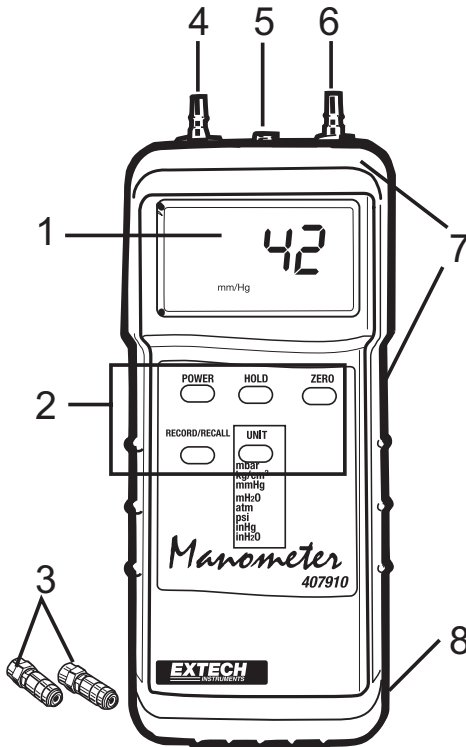

Basic Operation

Meter Power

This device uses a 9V battery for power. If the meter does not switch on when the POWER button is pressed or if the display shows **LBT**, replace the battery (refer to the Battery Replacement section later in this manual).

In order to conserve battery life, the meter has an automatic power off feature (after 10 minutes). To defeat this feature, access the RECORD mode by pressing the RECORD/RECALL button. In the RECORD mode, the meter will remain on until the user turns it off or until the battery weakens.

Unit of measure

Press the UNIT button to select the unit of measure. This meter offers eight (8) units of measure as listed below, in the specifications chart earlier in this manual, and on the face-plate of the meter.

Units	Displayed Symbol
MBAR	"m" at bottom of the LCD and "Bar" at the top
Kg/cm2	Kg /cm ²
mm of Hg	mm /Hg
m H ₂ O	m H ₂ O
Atmospheres	ATP
PSI	PSI
Inches of Hg	in/Hg
Inches of H ₂ O	inch H ₂ O

Zero Adjust and Offset function

Before use and without fittings attached to the meter, press the ZERO button to calibrate the meter's circuitry. The display should then indicate zero.

If it is desired to offset the meter's display, press the ZERO button while taking a measurement. Subsequent readings will be the difference between the current measurement and the measurement that was on the display when the ZERO button was pressed.

Fittings Connection

Connect tubing to the quick-disconnect fittings and then snap the supplied quick-disconnect fitting(s) to the P1, P2 (or both) input port(s). If both inputs are used (differential mode), the meter displays a positive pressure reading if the P1 pressure is greater than P2 and a negative reading if P2 is greater than P1.

MIN/MAX Record/Recall Mode

The Record/Recall function tracks the maximum and minimum readings for recall at any time.

1. Press the RECORD/RECALL button once. The REC indicator will appear on the display.
2. Press the RECORD/RECALL button again to view the highest (MAX) reading taken since the RECORD/RECALL button was first pressed. The MAX indicator and maximum reading will appear on the display.
3. Press the RECORD/RECALL button again, the MIN indicator and the minimum value will appear on the display.
4. To return to normal operation, press and hold the RECORD/RECALL button until the display indicators REC, MAX, and MIN disappear.

RS-232 PC Interface

The meter has a built-in RS-232 serial port for use with the optional PC Interface Data Acquisition Software/Hardware kit Model 407001.

Battery Replacement

When the low battery indicator **LBT** appears on the display or if the meter does not switch on when the **POWER** button is pressed, it is necessary to replace the battery.

To replace the battery:

1. Remove the meter's rubber protective jacket by stretching it over the bottom of the meter.
2. Pry open the battery compartment located on the back of the meter using a small coin or screwdriver.
3. Replace the 9V alkaline battery
4. Replace the battery compartment cover and the protective jacket.

Useful Conversions

Useful conversion Factors		
From	To	Multiplier
In of H ₂ O	In of Hg	0.07355
In of H ₂ O	Cm of Hg	2.54
mm of Hg	In of H ₂ O	0.03937

Calibration and Repair Services

Extech offers repair and calibration services for the products we sell. Extech also provides NIST certification for most products. Call the Customer Service Department for information on calibration services available for this product. Extech recommends that annual calibrations be performed to verify meter performance and accuracy.



Support line (781) 890-7440

Technical support: Extension 200; E-mail: support@extech.com

Repair & Returns: Extension 210; E-mail: repair@extech.com

Product specifications subject to change without notice

For the latest version of this User's Guide, Software updates, and other up-to-the-minute product information, visit our website: www.extech.com
Extech Instruments Corporation, 285 Bear Hill Rd., Waltham, MA 02451

Copyright © 2005 Extech Instruments Corporation

All rights reserved including the right of reproduction in whole or in part in any form.