

Accurate Thermal Systems - ThermCal400 Dry block calibrator stability


Stability at 100C

Stability over 40 minute period

0.011 Total Stability +/-

After allowing unit to stabilize for 20 minutes

0.009 Total Stability +/-

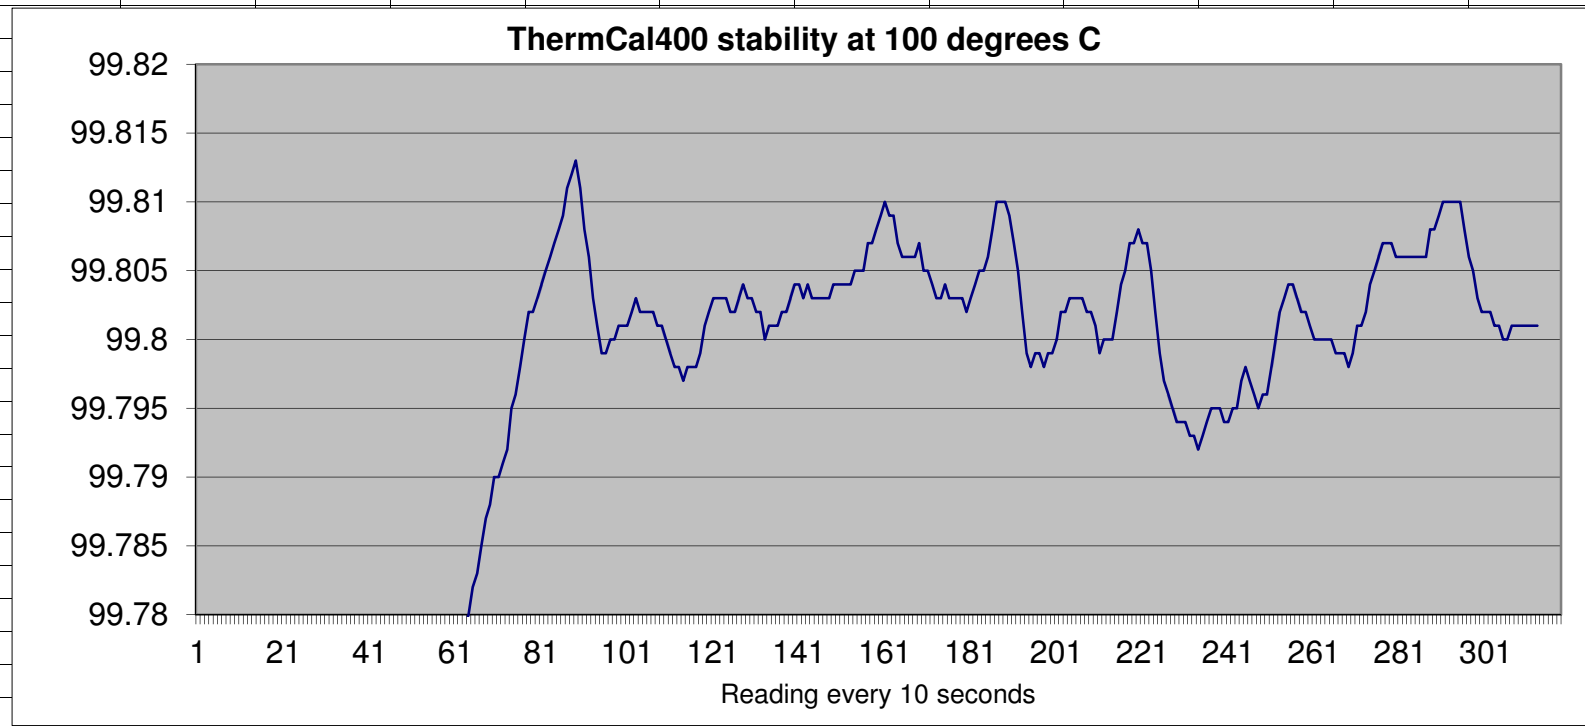

Stability at 300C

Stability over 52 minute period

0.025 Total Stability +/-

After allowing unit to stabilize for 20 minutes

0.013 Total Stability +/-

