

Technical Datasheet



VTE 02 (Ex)




Carrier-Frequency Pulse Amplifiers
with Single Pickup

Application

The VTE 02 are carrier frequency pickups for all ZHM, HM, SRZ and LFM. Due to the wide frequency range (0.5 to 5,000 Hz) they work with all sizes.

For applications in hazardous areas intrinsically safe versions with ATEX and IECEx certification for zone 1 and cCSAus certification for zone 0 and division 1 are available.

Technical Data

Supply Voltage U_B	10 up to 30 V DC, regulated 7 up to 30 V DC („U“, NAMUR operation) 5 up to 10.5 V („N“)	
Quiescent Current	< 1 mA	
Frequency Range	0.5 up to 5,000 Hz	
Ambient Temperature	-40 °C up to +80 °C [-40 °F up to +176 °F] (non Ex) -40 °C up to +60 °C [-40 °F up to +140 °F] (Ex, T4)	
Medium Temperature	Form K + R: -40 °C up to +120 °C [-40 °F up to +248 °F] ¹⁾ Form L + S: -40 °C up to +150 °C [-40 °F up to +302 °F] ²⁾	
Housing	Stainless steel as per DIN 1.4104 [AISI 430F] Option: 1.4404 [AISI 316L]	
Dimensions	See dimensional drawing (page 3)	
Ingress Protection	IP65	
Ex Protection	ATEX: II 2G Ex ia IIC T4 Gb IECEx: Ex ia IIC T4 Gb cCSAus: Class I, Div. 1, Groups A, B, C, D; T4 Ex ia IIC T4 Ga Class I, Zone 0 AEx ia IIC T4 Ga	
Electrical Connection ²⁾	M12 plug-in connector (5-pin, male, A-coded) 1 = $+U_B$ 2 = n.c. / NAMUR- („N“, „U“) 3 = 0 V (not „N“) 4 = Signal Push Pull (not „N“) 5 = n.c.	
	M16 plug-in connector (5-pin, male, A-coded) (option) 1 = $+U_B$ 2 = Signal Push Pull 3 = 0 V 4 = n.c. 5 = n.c.	
	MIL plug-in connector (3-pin, male, A-coded) (option) A = $+U_B$ B = 0 V C = output	

¹⁾ With a distance >25 mm between flow meter and electronic housing

²⁾ With a distance >65 mm between flow meter and electronic housing


³⁾ Other plugs or pin assignments on request.

Ex-Supply Data

Supply Circuit (pin 1 and 3) (version P, U)	Voltage	$U_i = \text{DC } 30 \text{ V}$
	Current	$I_i = 120 \text{ mA}$
	Power	$P_i = 850 \text{ mW}$
	Effective internal capacitance	$C_i = 8 \text{ nF}$
Signal Current Circuit Push/Pull (pin 3 and 4) (version, P, U)	Voltage	$U_i = 30 \text{ V}$
	Current	$I_i = 24.6 \text{ mA}$
	Power	$P_i = 185 \text{ mW}$
	Effective internal capacitance	$C_i = 8 \text{ nF}$

Ex-Supply Data Version „N“ NAMUR


Supply and Signal Circuit (pin 1 and 2)	Voltage	$U_i = \text{DC } 10.5 \text{ V}$
	Current	$I_i = 16 \text{ mA}$
	Power	$P_i = 40 \text{ mW}$
	Effective internal capacitance	$C_i = 8 \text{ nF}$

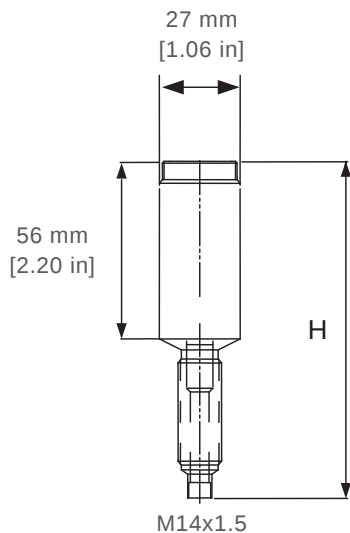Dimensional Drawing


Type	H
VTE 02 - K	110 mm (4.33 in)
VTE 02 - R	110 mm (4.33 in)
VTE 02 - L	149 mm (5.87 in)
VTE 02 - S	149 mm (5.87 in)

Output (short-circuit proof)


Push Pull

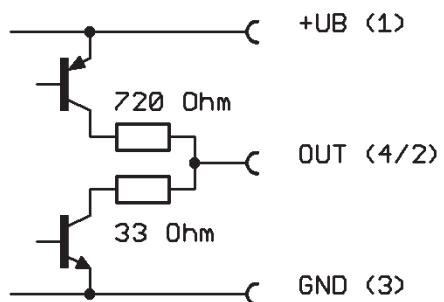


Open Collector

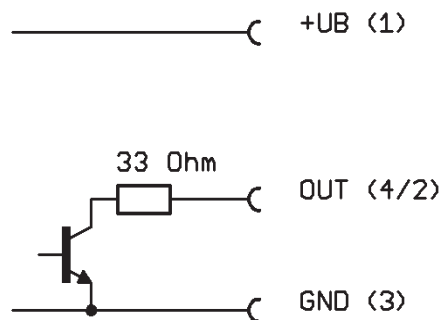

NAMUR

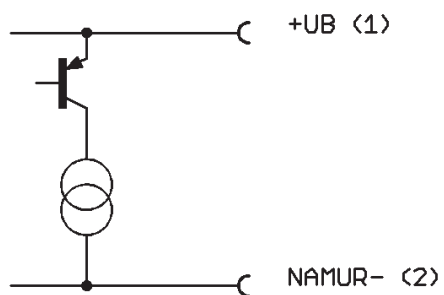

Push Pull + NAMUR

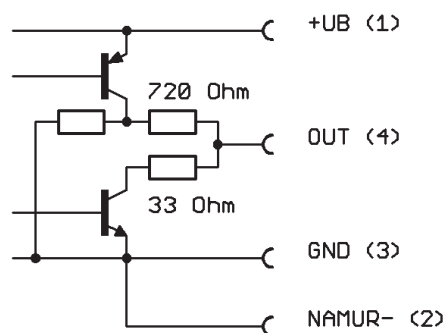

Ordering Code

	VTE02	-	X	-	X	-	X	-	X	
Pickup form										
ZHM 01/* - 04, HM series			K							
ZHM 01, SRZ Serie, LFM series			R							
ZHM 01/* - 07, HM series			L							
ZHM 01, SRZ , LFM series			S							
Output⁴⁾										
M16, Push-Pull					A					
MIL-5015 3-pin, Push Pull					D					
MIL-5015 3-pin, Open Collector					E					
M12, Push Pull					P					
M12, NAMUR					N					
M12, NAMUR + Push Pull					U					
Ex Protection										
No certification										
ATEX (II 2G Ex ia IIC T4 Gb), IECEx, cCSAus							Ex			
ATEX (II 3G Ex nA IIC T4)							Exn			
For custom specific options										01-99

Examples

VTE02-K-N-Ex	K-Pickup, M12, NAMUR, Ex certification ATEX, IECEx, cCSAus
VTE02-R-P	R-Pickup, M12 push-pull, no Ex

Safety Instructions

The following has to be adhered to:

- Installation instructions for electrical devices
Installation instructions for associated intrinsically-safe devices
The »Special conditions for safe use« as per EC-Type Examination Certificate
- The amplifier has to be installed in a way that the max. ambient temperature does under no circumstances exceed +60 °C [+140 °F].
- With cables care should be taken, that the max inductivity and capacity of the respective voltage or gas group are not exceeded
- Exceeding or falling below the regular measuring range will cause invalid frequency output signals.
- Shielded cables are to be used as connecting lines.
- Generally, supplied units have to be connected by an expert according to EMC stipulations.
- Disconnect power supply before making electrical connection.

⁴⁾ Other plugs or pin assignments on request.



Küppers Elektromechanik GmbH

www.kem-kueppers.com

info@kem-kueppers.com

KEM Headquarters

Liebigstraße 5
85757 Karlsfeld
Germany

T. +49 8131 59391-0
F. +49 8131 92604

info@kem-kueppers.com

KEM Manufacturing Center

Wetzeller Straße 22
93444 Bad Kötzing
Germany

T. +49 9941 9423-0
F. +49 9941 9423-23

production@kem-kueppers.com

KEM Sales

Liebigstraße 5
85757 Karlsfeld
Germany

T. +49 8131 59391-100
F. +49 8131 92604

sales@kem-kueppers.com

KEM Service & Repairs

Wetzeller Straße 22
93444 Bad Kötzing
Germany

T. +49 9941 9423-37
F. +49 9941 9423-24

service@kem-kueppers.com

*More distributors & partners can be found at:
www.kem-kueppers.com*